

GLOBUS
ITALIAN EXCELLENCE

ELECTROSTIMULATORS



User Manual

THE CHAMPION



CE
0476

DEAR CUSTOMER

**THANK YOU FOR CHOOSING A GLOBUS PRODUCT. WE REMAIN AT YOUR
DISPOSAL FOR ANY ASSISTANCE OR ADVICE YOU MAY NEED**



DOMINO s.r.l.
via Vittorio Veneto 52
31013 - Codognè - TV - Italy
Tel. (+39) 0438.7933
Fax. (+39) 0438.793363
E-Mail: info@globuscorporation.com
www.globuscorporation.com

Table of contents

THE CHAMPION

TECHNICAL FEATURES	4
Device.....	5
Technical features of the currents.....	5
Disposal of the device.....	6
Declaration of conformity	6
INTENDED USE	7
The risk class of the device is IIb.	7
EQUIPMENT	8
LABELLING AND SYMBOLS.....	10
Device.....	12
Panel and keyboard.....	14
Display and interface	15
INFORMATION SIGNALS.....	15
Compliance	15
PREPARATION TO THE USE OF THE DEVICE	15
Warnings before the use.....	16
How to connect the cables	17
Connection of the electrodes	17
Battery	17
Use of the water-proof case.....	18
Safety precautions	19
Contraindications	19
Side effects.....	20
USER GUIDE OF THE DEVICE.....	21
Program List menu	21

THE CHAMPION

“Last 10” Menu	23
“Treatments” Menu	24
“Programming” Menu	25
Advanced Menu	26
PROGRAM LIST.....	28
GENERAL NOTES ON ELECTRODE POSITIONING	36
ELECTRODE POSITION	39
ELECTRODE POSITION (TENS)	42
MICROCURRENT ELECTRODE POSITIONING	43
Muscular electrostimulation	44
Stimulation intensity	45
Tens	46
Microcurrents	47
Ionophoresis	47
MAINTENANCE AND CLEANING.....	48
Device.....	48
Battery	48
Accessories	48
WARRANTY	49
FAQ	50

TECHNICAL FEATURES

Device

Size:	160x99x35.4 mm
Weight:	404 g
Case:	in Food Grade ABS
Protection level:	IP20 + IP02

Use Conditions

Temperature:	from 0°C to 35°C
Maximum relative humidity:	from 15% to 93%
Atmospheric pressure:	from 700 hPa to 1060 hPa

Storage and transport conditions

Temperature:	from -10°C to 45°C
Max.relative humidity:	30% - 75%

The values represent the limits allowed if the product or the accessories are not in their original package.

Technical features of the currents

EMS and TENS:

Channels available:	Channels 1-2-3-4
Constant current:	Yes
Intensity:	0-120 mA with 1000 Ohm load
Wave form:	Rectangular, biphasic, symmetrical, compensated
Working frequency:	0.3-150 Hz
Recovery frequency:	0.3-150 Hz
Pulse amplitude:	50-450 µs
Working time:	from 1 to 30 seconds
Recovery time:	from 0 to 1 minute
Frequency mod. range:	continuous variation from 1 to 150 Hz
Min. modulation time:	3 seconds
Amplitude modulation range:	continuous variation from 50 to 450 µs

Microcurrents:

Channels available:	Channels 1-3
Constant current:	Yes
Min. frequency:	5Hz
Max. frequency:	200Hz
Min. Intensity:	0 µA/1000 Ohm Step 10 µA

THE CHAMPION

Max. Intensity: 800 μ A/1000 Ohm
Amplitude value: included between 1 and 250 μ seconds

Ionophoresis:

Channels available: Channel 1
Constant current: Yes
Min. Intensity: 0 mA/1000 Ohm
Max. Intensity: 10 mA/1000 Ohm step 0.1 mA/1000 Ohm
Min. time: 1 minute
Max. time: 99 minutes

Charger

Brand: FLO
model: DKT-088-0200-EU
Input: 100-240V~ 50-60Hz 0.07A Max
Output: + 8.8 V --- 0.2A Max
Polarity: 

Battery

Battery pack: Ni-MH 7,2 V 1,8 Ah

Disposal of the device

Do not throw the device or parts of it into the fire; dispose of the product in the specialized centers and respecting the regulations in force in your Country. When the product has to be disposed of, the user can give it back to the retailer when purchasing a new device.

A correct separate waste collection or the compliance with the above-mentioned prescriptions contribute to avoiding possible negative effects on the environment and the health and promote the reuse and/or recycle of the materials of which the device is composed. The illegal disposal of the product entails the application of administrative fines according to applicable regulations.

Declaration of conformity

The device has been manufactured in compliance with applicable technical standards and has been certified, in compliance with Directive 93/42/EEC as amended by directive 2007/47 on medical devices, by the Notified Body Kiwa Cermet Italia, Via Cadriano 23, 40057 Granarolo Dell'Emilia (BO) Italy (n. 0476), in order to ensure product safety.

INTENDED USE

The estimated usable life of the product is 5 years. It is advisable to return the device to the producer and/or authorized center to perform security and maintenance checks every 2 years. The number of treatments depends on the battery charge.

The risk class of the device is IIb.

The device is intended for:

- Antalgic electrotherapy through peripheral nervous system stimulation;
- Muscular electrostimulation in order to reduce atrophy, spasticity and to increase the muscular power.


The electrostimulators are designed to be used in the following operating environments:

- domestic environment;
- clinics;
- physiotherapy centers;
- rehabilitation in general;
- pain treatments in general;
- for aesthetic and sport purposes (CE0476 does not refer to non-medical treatments).

The use of this equipment is allowed to the patient (appropriately informed of the conditions of use of the apparatus) and the medical staff.

The user of these devices must be competent to stand trial and must be over 18 years old.

EQUIPMENT

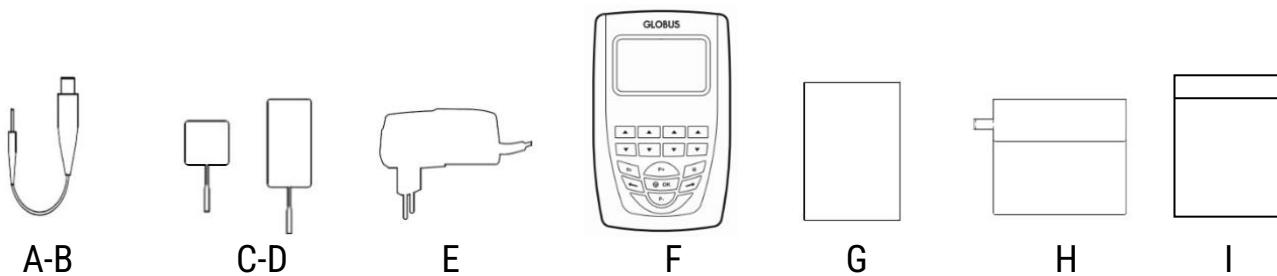

The electrostimulation device is supplied with all the necessary cables and electrodes; therefore, when you open the package, check that the basic equipment is complete. If some elements are missing, contact your authorized retailer immediately.

Check that the device and the electrodes are intact.

- A. 4 colored connection cables for electrodes (for EMS, TENS treatment)
- B. 2 gray cables (for microcurrent and ionophoresis treatments)
- C. 4 self-adhesive, re-usable electrodes (50 x 50 mm)
- D. 4 self-adhesive, re-usable electrodes (50 x 90 mm)
- E. Charger
- F. Device
- G. User manual
- H. Carrying bag
- I. Waterproof case

Equipment description

REF G0464 - Electrodes Myotrode Plus (50x50 mm). Package with 4 adhesive electrodes. Electrodes can be used multiple times on the same patient. We recommend the use of these electrodes for small surfaces such as upper limbs, calves, cervical area...

REF G0465 - Electrodes Myotrode Plus (50x90 mm). Package with 4 adhesive electrodes. Electrodes can be used multiple times on the same patient. We recommend the use of these electrodes for large surfaces such as thighs, abdomen, gluteus...

Accessories that are not included in the equipment (to be purchased separately)

The device can be combined with optional accessories (for further info and technical features, please visit our website www.globuscorporation.com). In order to purchase these accessories, please contact your dealer.

THE CHAMPION


REF	Name	Description
G1156	Motor point pen	It helps finding the best positioning of the electrodes
G1309	G-trode Handpiece	Bipolar G-PULSE head
G0479	Kit conductive elastic bands for thighs	Kit conductive elastic bands for thighs Bands can be used instead of electrodes, and are recommended for aesthetic and beauty treatments.
G0480	Kit conductive elastic bands for thighs and arms Fitness Top	Kit conductive elastic bands for thighs and arms Bands can be used instead of electrodes, and are recommended for aesthetic and beauty treatments.
G0487	Fast Band	Abdominal band for treatment on abdomen, gluteus and back - 98 cm
G0489	Fast Pad	Special reusable electrodes, specifically suitable for aesthetic treatments on thighs and gluteus.
G0488	Fast Body kit	fast band + fast pad
G0890	Medium ionophoresis electrode	Carbon electrode + pouch 50x50 mm
G0885	Big ionophoresis electrode	Carbon electrode + pouch 60x85 mm
G0439	Kit 2 splitting cables	This accessory is used to split the cables in order to use more electrodes at the same time.

LABELLING AND SYMBOLS




	It refers to the manufacturer
	Warning The device emits current values over 10 mA o 10V
	Keep the device dry
	This symbol indicates that the device complies with the directives on medical devices (93/42/EEC 47/2007/EEC). The number of the notified body is 0476.
	It indicates that this is a class II device.
	It indicates that this device has BF-type applied parts.
	WEEE symbol (Waste of Electrical and Electronic Equipment). Recycling symbol. The WEEE symbol used for this product indicates that it cannot be treated as a household waste. The proper disposal of the product will contribute to protecting the environment. For further information on the recycling of this product, please contact the concerned office of your local body, the household waste management company or the store where the product was purchased.
	It indicates that the product has been designed in compliance with the directive 2011/65/EEC
	It informs the operator that s/he must read the manual before using the device.
	It informs the client of the compulsory conduct
	It indicates the ideal temperature for the storage and transportation of the product.
IP20	It indicates water protection

THE CHAMPION

Model	It indicates the battery charger model
PRI	Input electric features of the battery charger
SEC	Output electric features of the power supply
Nerve and Muscle stimulator	It indicates the device type
Input power	Input electric features of the device for battery charging
Input battery	Features of the electric power supply from internal battery
Output	Output, indicates the maximum value of current emitted by the device
SN	It indicates the serial number of the device.
Internal battery	Indicates the features of the battery pack inside the device
	It refers to the expiry date of the product
LOT	It refers to the production lot
	It refers to the manufacturing date.
	It indicates the pressure of the environment in which the device and the accessories are transported and stored.
	It indicates the humidity of the environment where the device and its accessories are used and stored
RH	It indicates the percentage of storage humidity

THE CHAMPION

Device

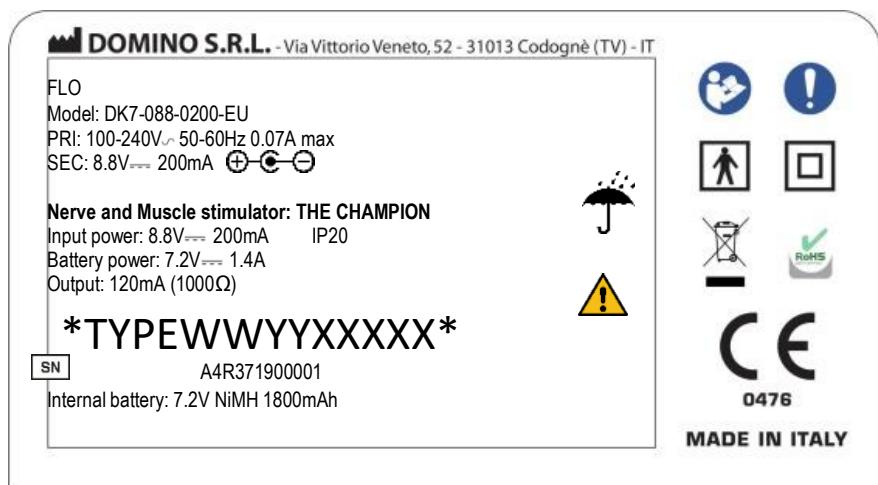

SN The first 4 digits of the serial number indicate the week and year of manufacture of the device you purchased (for example, if the code is *** 2319 ****, it means that the device was manufactured in week 23 of 2019).

Electrodes

	It indicates the dimensions of the electrode
	It indicates the number of electrodes contained in the package
REF	It indicates the product code
CE	It refers to product certification and indicates that it complies with directive 2001/95/EC updated as 2014/357/EU
	It indicates the storage temperature of the electrodes




- Clean and degrease the skin.

THE CHAMPION

- Do not apply the electrode on wounds or injured skin.
- Connect the cable connector to the electrode connector.
- Remove the electrode.
- Apply on the skin.
- Start the program.
- At the end, turn off and put the electrode back in the package.
- Electrodes are for personal use.
- Do not remove the electrode by grabbing the connector.
- Electrodes should not touch each other.
- Do not apply the electrodes on the temples, the neck and in a transthoracic way.
- Do not leave the electrodes in the car.

THE CHAMPION


Panel and keyboard

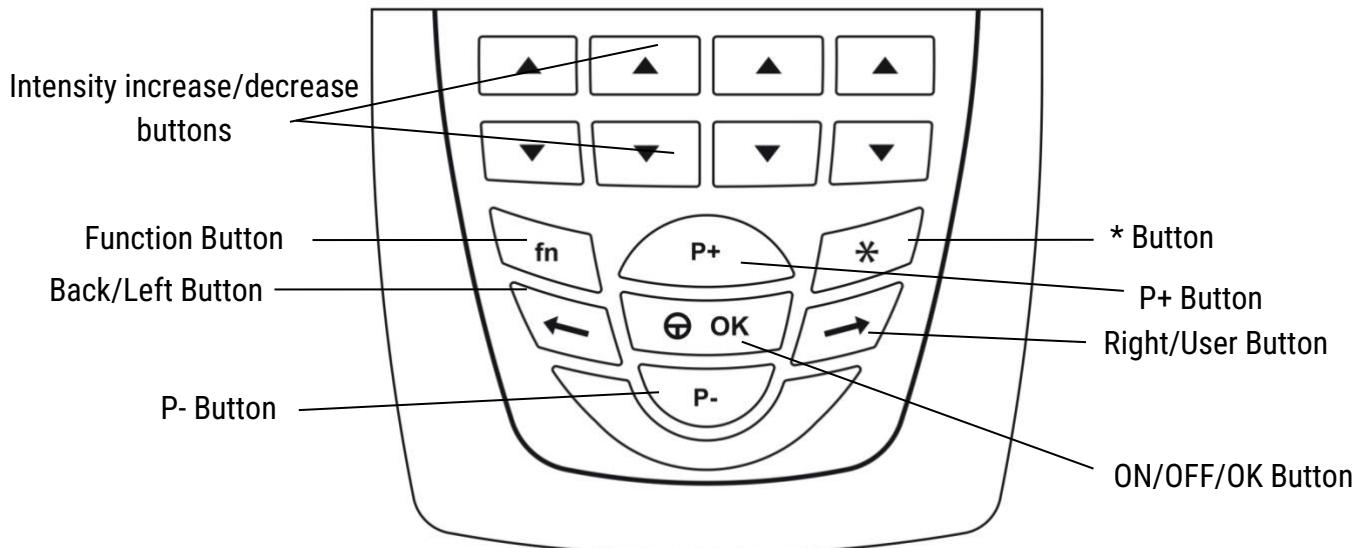

NOTE: when the 3" message appears, it means that holding the button down for 3 seconds activates the function.

ON/OFF/OK BUTTON	It confirms the selection. It pauses the running program. 3" = On/Off.
LEFT/BACK Button	To scroll the selection left. To go back to the previous selection. 3" = It returns to the previous phase while the program is running.
P+ Button	It moves the selection upwards. It increases the intensity of the 4 channels simultaneously, while a program is running
P- Button	It moves the selection downwards. It increases the intensity of the 4 channels simultaneously, while a program is running
RIGHT/USER button:	It moves the selection to the right. 3" = It moves to the next phase, while a program is running
* Button	It starts and stops the contraction while "Action Now" programs are running (where "Action Now" programs are included).
Fn (Runtime) button	If pressed together with other buttons, it permits the user to modify their function. Moreover, it selects Runtime mode (editing time, frequency and amplitude)
Intensity button	It increases/decreases the stimulation intensity of the corresponding channel.

Display and interface

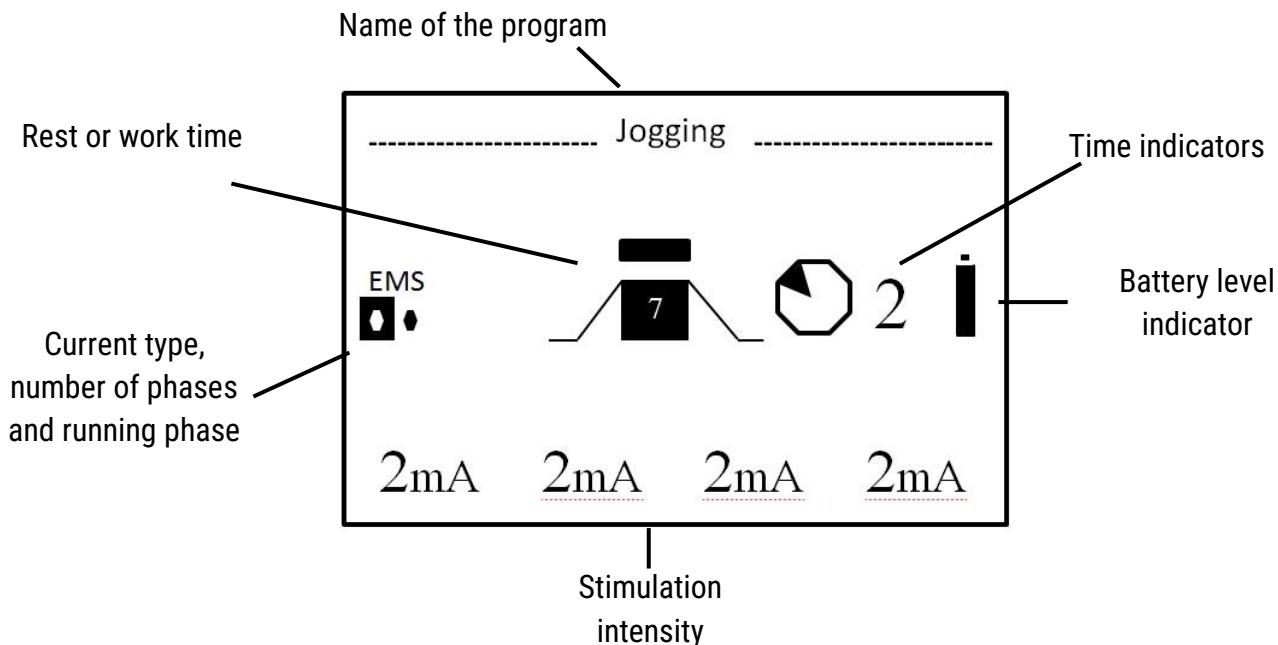

INFORMATION SIGNALS

Compliance

Certifications: CE MDD certificate.

The sound and acoustic signals are in compliance with the 60601-1-8 directive.

Meaning of the signal "Electrode error"

If one or more cables are not duly connected to the mains, or if cables for microcurrent are erroneously used to run an EMS program, the following signal will appear on the display: "Electrodes error".

PREPARATION TO THE USE OF THE DEVICE



For maximum safety, the device must be used following the rules and the limitations of the user manual.

The manufacturer declines all responsibility with reference to a different use from what is indicated in this manual.

The full or partial reproduction in any form and by any electronic or mechanical means of the texts and/or pictures contained in this manual without the written authorization of the manufacturer is forbidden.

Treatments should not be performed on skin lesions.

If the package, the cable or the connector of the power supply show signs of wear or damage, replace it instantly.

The device should be connected to the mains with its power supply; before doing so, make sure that the power system complies with the directives in force in your country. Make sure that the power supply will be easily unplugged.

The use of muscle stimulation programs referred to the treatment of urinary incontinence can be used exclusively for the treatment of urge, stress and mixed incontinence.

Warnings before the use

For the stimulation part, the device works with batteries only. On the contrary, navigation throughout the menu is available also during recharge.

Do not use this device simultaneously with other electronic devices, especially if they maintain vital functions. In case it is necessary to use the device nearby or on other devices, make sure it works properly, please refer to the chapter EMC accompanying documents.

- It is recommended to read carefully the entire operating manual before using the unit; keep carefully this operating manual.
- The device is capable of delivering current values exceeding 10mAms.
- Before each use always check the integrity of the device. This is a fundamental requirement for carrying out the therapy; do not use the device if the buttons or the cables are defective or malfunctioning.

It should be used only by people over 18 and, in any event, who are able to understand and take action.

- It should not be used for purposes other than transcutaneous neurostimulation.
- it must be used following the indications and under the strict control of the physician or qualified physiotherapist.
- The device must be used with the transcutaneous neurostimulation electrodes suitable for this use.
- The device must be kept out of the reach of children.
- With its current, it can disturb ECG monitoring devices.
- It must not be used in a transthoracic mode as it could cause cardiac arrhythmia by superimposing its frequency to that of the heart. (Do not perform the treatment on the chest and the back simultaneously)
- If there is any health problem, it must be used only after consulting a physician.

THE CHAMPION

- A simultaneous connection of a patient to a high frequency electrosurgical device can cause burns near the electrodes of the stimulator and therefore the stimulator may be damaged.
- Once you have turned the device on, make sure the display shows the software version and the device model: it means that the device is working and ready to be used; If it doesn't, or the display does not show all the segments, turn it off and on again. If the problem persists, contact the service center and do not use the device.
- The sudden shutdown shortly after the starting indicates a low battery level. Recharge as reported in the section "HOW TO CHARGE THE BATTERIES".

How to connect the cables



In order to connect the cables to the device, plug the connectors into the intended inlets on the top of the unit (see picture). **Cables should be inserted with grooves downwards.** The inlets are placed exactly under the corresponding channels.

NOTE: for EMS and TENS currents use indifferently the 4 channels with colored cables.

NOTE: for microcurrents and handpiece for face use channel 1 or 3.

NOTE: for ionophoresis, use channel 1 only with gray cables.

Connection of the electrodes

Take the electrodes from the original packaging; all new electrodes have a sealed packaging. Ensure that the device is off. To start, connect the two plugs of the cables to the electrodes, then remove the electrodes from their place and put them on the skin. To place the electrodes correctly, see the images at the end of this manual.

After the use, place the electrodes back in their specific place.

WARNING: do not unplug the electrodes if the device is operating.

Battery

The device is equipped with a nickel-metal hydride rechargeable battery pack (7.2V, 1.8Ah), which has a high performance and no memory effect.

The battery has an estimated life of 6 months in case it is not used. The number of cycles (discharge and recharge) depend on the type of stimulation and on the frequency

THE CHAMPION

treatments are executed. The device is supplied with charge indicator; it is advisable to recharge when it indicates ¼. In case after recharge the number of executable treatments is reduced, the battery must be replaced.


How to charge the batteries



After turning the electrostimulator off and removing the electrodes, connect it to the charger supplied by inserting the connector into the specific socket (see picture above). Never use a charger that is different from the one supplied with the device. Please contact our customer care to replace the battery pack.

Use of the water-proof case

To ensure the IP 02 water-proof level in home use, put the device into the water-proof case included in the equipment. Then pressure-close the zip and let the cables come out of the upper corner of the case. Use a twist tie to seal the closure on the corner. Complete the insertion as in the picture below.

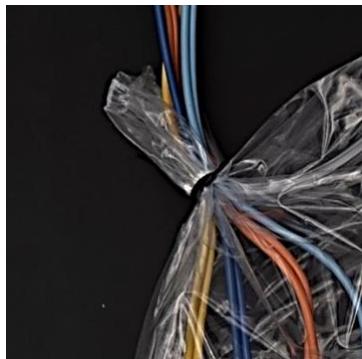

Safety precautions

While using the electrostimulator, some warnings should be followed:

- In the case of damaged cables, they must be replaced with original parts and not used anymore.
- Only use Globus marked electrodes.
- Great attention has to be paid when current densities exceed 2mA/cm² (effective value) for each electrode.

The device must be kept out of the reach of pets, as they could damage the device and contaminate the electrodes and other accessories with parasites.

- The cables of the electrostimulator should not be wrapped around people's neck to avoid any risk of strangulation and suffocation.
- Keep out of the reach of children who may accidentally swallow small detachable parts of the device (for example the support feet).
- Mobile and fixed radio communication devices might affect the functioning of the electromedical device: see the tables attached to this manual. Please refer to the chapter EMC accompanying documents.

Contraindications

The device should not be used in the following cases:

- Stimulation of the urogenital apparatus, in case of extra-ureteral incontinence;
- Stimulation of the urogenital apparatus, in case of incontinence due to evacuation disorders;
- Stimulation of the urogenital apparatus, in case of chronic urinary retention, in the upper urinary tract
- Stimulation of the pelvic floor in presence of a complete peripheral denervation;
- In case of actual or alleged tumour formation, consult the oncologist
- Pains with unknown etiology.
- Stimulation on areas with sores and dermatological diseases.
- Stimulation on areas with acute traumas
- Pregnancy;
- Presence of severe cognitive deficiencies that do not permit the patient to communicate or perceive pain or discomfort;
- People whose sensitivity to health and/or pain is diminished due to surgery interventions, anesthesia, ionizing radiations treatments, diabetes, etc.;
- Presence of severe pathologies on main organs
- Presence of neurological diseases.

Do not use the device on the following parts pf the body:

- Eyes zone;
- Stimulation of the anterior neck (carotid sinus).
- Brain region
- Near body areas with metallic implants or infra-tissue metals (e.g. prostheses, osteosynthetic devices, coils, screws, plates), when using monophasic currents such as interferential and continuous currents (ionophoresis).
- In presence of pacemaker and active implantable medical devices.

Patients suffering from a total/subtotal prolapsed uterus/vagina must be evaluated by a doctor and stimulated with extreme caution.

Patients with urinary tract infections should be treated for these symptoms before starting use the electrostimulator.

It is also recommended to use the device with caution in case of capillary fragility, as excessive stimulation may cause a further break of capillaries.

Side effects

Skin irritation may occur in subjects with high skin sensitivity.

In case of allergic reaction to electrode gel, suspend the treatment and contact a specialist.

If during the treatment signs of tachycardia and extrasystole appear, suspend the treatment and contact your physician.

USER GUIDE OF THE DEVICE

For a correct use of the device, proceed as follows:

- connect the cables to the inlets on the unit;
- connect the electrodes to the specific connectors at the end of the cables;
- place the electrodes on the skin.

Start up

Hold the On/Off (OK) button down for about 3 seconds until a sound signal is heard.

The model name and software version will appear with a number on the lower right.

Depending on the model, different entries will appear. Use the P+ and P- buttons of the joypad to choose your function in the main menu:



Program List menu

When selecting the "Program list", the following areas are displayed depending on the model:

- SPORT
- SPECIAL SPORTS
- FITNESS-PHYSICAL SHAPE
- BEAUTY-AESTHETICS
- MEDICAL CURRENTS
 - MICROCURRENTS
 - IONOPHORESIS
 - ANTALGIC PAIN
 - REHABILITATION
- ACTION NOW
- SERIAL SEQUENTIAL STIMULATION
- G PULSE

Program selection

- Area selection:

Use the P+ and P- buttons to select the desired area and press OK to confirm.

Press the LEFT (Back) button to return to the previous screen.

- Program selection.
- Body part selection (where it is present)

How to start the program

When the program is selected, the display will show the following entries:

- Start;
- Electrode position;
- Save to Favorites (see Favorites Menu)
- Save to Treatments (see Treatments Menu)
- Continue with 2+2 (see 2+2 mode)

To start the program press Start and increase the intensity of the channels in the screen that follows.

How to increase and decrease intensity

To increase/decrease the intensity of single channels, press Up and Down on the corresponding channel.

Syncro Stim function

Press P+ or P- to increase or decrease the intensity of all the channels.

Runtime function (how to change the working phase parameters)

After starting the program, the following parameters can be edited:

- Time
- Frequency
- Amplitude

Press Function to edit the parameters of the phase in progress: a new screen will appear and display the phase time.

Press P+/P- to edit the time.

Press Fn or wait for 5 seconds to confirm the new time settings.

Press LEFT/RIGHT and repeat the above-mentioned procedures to edit the other parameters.

Display during program execution

While the program is running, the screen displays the name of the program (at the top), the number of total phases and the phase in progress, the remaining time of the phase in progress and the type of the wave used (EMS, TEN, MICRO...). When performing an intermittent treatment, the screen displays the countdown indicator and the work and rest phases.

How to pause the program

To pause the program, press the "Ok" button on the joypad. Press OK again to return to the program.

At the start of every treatment or after the interruption of a protocol, the device restarts from a 0 intensity value.

How to stop the program

Press OK for three seconds to stop the program before its end.

How to skip a phase

Hold RIGHT down for 3" to pass on to the following phase before the conclusion of the phase in progress.

Hold LEFT for 3" to return to the previous phase.

"Last 10" Menu

The electrostimulator keeps track of the last 10 executed programs. In this way, they are available for a very simple and fast execution.

The recording takes place automatically at the end of the execution of a program. If the memory is full, the older program is automatically deleted.

When you turn the device on, select "Last 10" and confirm with OK.

With the P+ and P- keys of the joypad, select the program you want to run (if there is no program in this menu you will read "EMPTY").

After confirming the selection 3 entries will appear:

- a - Start
- b - Electrode placement (electrode placement)
- c - Delete from the list

a - After selecting "Start", it is possible to choose whether to run the program in automatic or normal mode. Press OK to activate the Automatic mode. Press any Increase Intensity button to run the program in Normal mode.

The message AUTO appears on the display when the "automatic" function is activated.

Automatic function (AUTO STIM)

Available only for EMS and TENS currents.

The "AUTO STIM" function allows to execute automatically a program that has already been executed, without having to set the intensity. Intensity values will be set automatically, restoring the values used during the latest execution of the same program.

The "AUTO STIM" function can only be activated by the programs stored inside "Last 10" memory in the menu.

NOTE:

- To run a program in "AUTO STIM" mode, it is strictly necessary that the electrodes of each channel are placed in the same position and muscular group (or body part) as in the latest execution of the program. Intensity values are specific for each channel.
- If the "AUTO STIM" function is used, each user has to use the machine always with his/her USER code.

Press any intensity button to exit the "AUTO STIM" mode.

-Choose "Electrode placement" you will have a guide to the correct positioning of the electrodes.

For further information on the electrode position, see the illustrated guide at the end of this manual.

-Select "Delete from the list" to remove the program from the "Last 10" list.

The "Last 10" memory refers to a specific user. The "USER SELECTION" (Multi-users) function allows the creation of a "Last 10" memory (up to 10 users plus the default user, defined as USER 0).

"Favorites" Menu

The "Favorites" menu allows you to save your most used programs on a special memory up to 15 for each user. In order to save a program, enter the "Program List" menu and choose the program you want to store. Before the execution, select "Save to Favorites" and confirm with OK.

The selected programs are easily available inside the "Favorites" menu.

NOTE: In Mode 2+2, it is not possible to store in Favorite programs.

"Treatments" Menu

The "Treatments" menu (**Stim Lock**) allows the user to lock the device and ensure that only the treatments saved with the "Save to..." function in the screen-page before the execution of the program are performed.

This feature is conceived for the rental of the device to inexperienced users and/or patients who have to perform only certain protocols determined by the professionals.

Stim Lock function activation

Press and hold the buttons fn + →(RIGHT button) for at least 3 seconds until the area where treatments have been saved appears.

After the Stim Lock is activated, the device will have a limited functionality.

Stim Lock function deactivation

Hold the fn + ← (SX) buttons down for at least 3 sec. and in any case until the main menu appears.

NOTE: If you turn the device on and the main menu does not appear check that the Stim Lock function is not on.

Try to deactivate it.

If the problem persists contact the customer care service.

“Programming” Menu

The electrostimulator offers the possibility of creating and modifying new programs. This makes the device flexible and adaptable to your needs.

From the "Programming" menu you can create new programs (when the message "EMPTY" appears) and perform those already customized. These can be modified at any time (see "Program modification").

The programs created in the "Programming" menu are unique for all "USERS" and are not stored neither in "Last 10" nor in "Favorites".

How to create a new program

With P+ or P- buttons, select the spot where you want to create the program and confirm with OK.

How to insert the name of the program

Use the Left and Right buttons to select the letters and confirm with the OK button. In order to delete a letter select "Del". After inserting the name of the program, select "Continue".

Setting of the parameters

STEP 1 Press "P+" or "P-" to select the stimulation type.

STEP 2 Press "P+" or "P-" to select the number of phases of the program.

STEP 3 After the number of phases is programmed, a series of screens will give the possibility of selecting the parameters. Use P+ and P- buttons to make your choice.

The previously described steps are the same for all the programs.

If the program presents more phases, the next required phase will be automatically proposed at the end of the insertion of a phase.

N.B. The programmed stimulation types vary according to the model.

Editing or deleting a program

In the "Programming" menu, you can edit or delete programs that you previously stored in memory.


Press "fn" + "P+" to edit and "fn" + "P-" to delete.

THE CHAMPION

NOTE: it is not possible to program mixed multiphase programs (e.g. a EMS+TENS program).

Advanced Menu

The advanced menu includes the following entries:

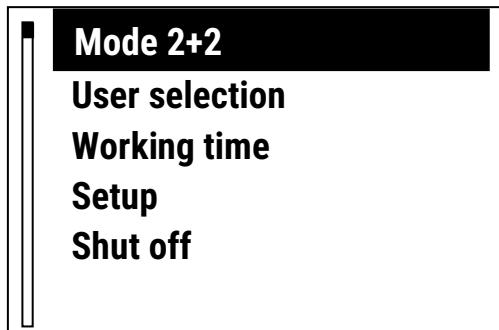

Mode 2+2

The device permits the simultaneous execution of two different programs (EMS or Tens), permitting the treatment of two patients or two muscular groups at once. How to set multiple treatments:

There are two options to run two programs simultaneously:


- Select the "2+2 mode" from the "Advanced" menu*
- From the Program list menu**

*Select "Last 10" from the main menu and press OK to confirm.

Select the area and the name of the first program. At this point, it is possible to select the area and the name of the second program.

**From the menu "Program list" choose the area and the desired program. At this point, select "Continue with 2+2" and choose the second program.

Note: During the execution of the 2+2 mode, the following screen will appear:

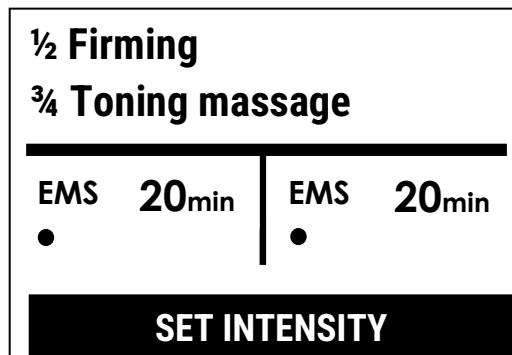

The program on the left side of the screen will work on channels 1 and 2, while the one on the right side on channels 3 and 4.

User selection

THE CHAMPION


It allows to use the special menus ("Last 10", "Favorites") in a personalized way. In order to gain access to favorite and "Last 10" programs, it will be sufficient to select one's USER. The programs stored in this area can be used only by that specific user. NOTE: Every time the device is turned on, the last user will be displayed.

Working time

It indicates the total time the device has been used for stimulation treatments.

Setup

By selecting the Setup menu, the following screen will appear:

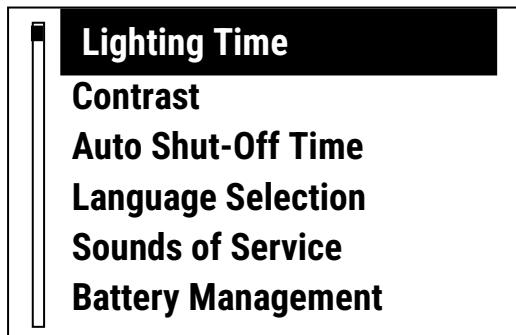

- **Function "Lighting Time"**

Press P+ and P- to modify the backlight time in stand-by mode.

- **"Contrast" function**

Press P+ and P- to modify the display contrast.

- **"Auto shut off timer" function**

It permits the user to choose the inactivity period after which the device automatically shuts down. Press P+ and P- to set the time in minutes.

- - **"Language selection" function**

Press P+ and P- to choose one of the 5 available languages. Confirm the selection with OK.

- **"Service sounds" function**

It allows to enable (YES) or disable (NO) the acoustical beeps the device emits.

- **"Battery Management" Function**

PROGRAM LIST**Sport Program List**

Capillarization
Decontracting
Warm-up
Pre-competition warm-up
Active recovery
Maximum strength
Endurance strength
Explosive strength
Reactivity
Post-competition recovery
Hypertrophy
Aerobic endurance
TOTAL 53

NOTE: some programs are divided according to body areas.

CE0476 does not refer to non-medical treatments.

Special Sports program List

SOCCER	VOLLEYBALL	RUGBY
Specific strength 3 levels	Maximum strength	Maximum strength
Speed endurance 3 levels	Explosive strength	Explosive strength
CROSS COUNTRY SKIING	Reactivity	Speed endurance 2 levels
Endurance strength 3 stages	Shoulder prevention	TRIATHLON
Endurance 3 stages	GOLF	Aerobic exercise 3 levels
RUNNING	Specific strength 3 levels	Endur. strength 3 stages
Aerobic 3 stages	Shoulder strength 3 levels	SAILING
SWIMMING	MARTIAL ARTS	Endurance strength
Endurance strength	Explosive strength	Aerobic exercise
Aerobic exercise	Reactivity	TENNIS
BIKE		Specific strength 3 levels
Aerobic exercise 3 levels	TOTALE: 90 programmi	

NOTE: some programs are divided according to body areas.

CE0476 does not refer to non-medical treatments.

Fitness-Physical Shape Program List

Firming

Bio-Pulse firming

Sculpting

Bio-Pulse sculpting

Toning

Mass Building

Body sculpting

Definition

Jogging

Anaerobic fitness

Aerobic fitness

Cramp prevention

TOTAL 58

NOTE: some programs are divided according to body areas.

CE0476 does not refer to non-medical treatments.

THE CHAMPION

Beauthy-Aesthetics Program List

Drainage
Bio-pulse drainage
Lipolysis
Bio Pulse relaxing massage
Toning massage
Energizing massage
Connective massage
Swollen arms
Face capillaries
Definition
Lifting effect
Skin tone improvement
Post-pregnancy drainage
Post-pregnancy lipolysis
Post-pregnancy firming
Breast firming
Breast sculpting
Figure
TOTAL 60

NOTE: some programs are divided according to body areas.

CE0476 does not refer to non-medical treatments.

Medical currents – Microcurrents Program List

The following programs are medical

Epicondylitis
Scapulohumeral periarthritis
Muscle restoration
Contusion
Edema
Skin ulcer
Sciatica
Lumbago
Brachial neuralgia
Acute pain
Articular pain

THE CHAMPION

Stiff neck
Whiplash
Cervical spondylosis
Shoulder sprain
Carpal tunnel
Knee sprain
Osteoarthritis
Ankle sprain
Achilles tendon inflammation
Patellar tendon inflammation
Rotator cuff inflammation
Tendon inflammation
TOTAL 23

Because of the presence of clinical programs, this product is a medical device. Therefore it is certified by the KIWA CERMET ITALIA S.P.A. Body n°. 0476 according to 93/42/CEE directive for medical devices. The certification covers clinical applications.

NOTES ON THE USE OF MICROCURRENT PROGRAMS

This paragraph refers to the use of microcurrent programs.

The microcurrent programs differ from normal TENS and EMS programs as follows:

- While conventional electrostimulation (e.g. TENS) uses current in the milliamperes range, microcurrent electrostimulation uses currents in the microampere range that are imperceptible by humans. During Microcurrents programs, **it is normal that the user does not discern any stimulation.**
- When running a Microcurrents program, **use exclusively the special gray cables connected to the outlets of channels 1 and 3.** If the cables are not connected or are of the wrong type, it will not be possible to start the program. Check the connections and the cables.
- **The Microcurrents programs have prefixed intensity levels**, therefore it is not necessary to set them. When a Microcurrent program is activated, the electrostimulator automatically brings the intensity to the correct level. This value should not be altered during the execution of the program.
- The Microcurrents programs cannot be run in the "2+2 mode" with multiple treatments. If one tries to select a Microcurrents program in "2+2 mode", the electrostimulator will emit an error tone.

If, according to your therapist, you wish to modify the treatment protocol altering the intensity, press and hold the UP and DOWN button for 3 seconds.

THE CHAMPION

Medical currents-Pain Antalgic (Tens) Program List

The following programs are medical

Menstrual pain
Modulated antalgic Tens
Scapulohumeral syndrome
Endorphinic Tens
Chronic pain
Muscle pain
Chronic lumbago
Cervical pain
Bursitis-tendinitis
Osteoarthritis
Knee pain
Conventional antalgic Tens
Total 12

Because of the presence of clinical programs, this product is a medical device. Therefore it is certified by the KIWA CERMET ITALIA S.P.A. Body n°. 0476 according to 93/42/CEE directive for medical devices. The certification covers clinical applications.

Medical currents-Rehabilitation Program List

The following programs are medical

Quadriceps atrophy
Recovery after ACL surgery
Shoulder subluxation
Total 3

Because of the presence of clinical programs, this product is a medical device. Therefore it is certified by the KIWA CERMET ITALIA S.P.A. Body n°. 0476 according to 93/42/CEE directive for medical devices. The certification covers clinical applications.

Incontinence program list (inside the Rehabilitation area)

The following programs are medical

Mixed incontinence

THE CHAMPION

Stress incontinence

URGE incontinence

TOTAL 3

Because of the presence of clinical programs, this product is a medical device. Therefore it is certified by the KIWA CERMET ITALIA S.P.A. Body n°. 0476 according to 93/42/CEE directive for medical devices. The certification covers clinical applications.

Type

The urology programs require the use of specific endovaginal and endorectal electrode probes, certified according to the Directive for Medical Devices 93/42/EEC. These are bipolar probes with a 2-mm female adapter which attaches to 2-mm male cables.

Warnings

Urological electrostimulation is a medical application, which must be carried out under medical supervision.

Use

To correctly use the probe electrode, follow the instructions provided by the manufacturer and given by the physician.

Maintenance

For cleaning, sterilization and disinfection, refer to the manufacturer's instructions.

Suggestions

In case of deterioration of the probe electrode, replace it immediately.

Medical currents – Ionophoresis Program list

The following programs are medical

Ionophoresis

TOTAL 1

The home user can use the ionophoresis treatments only after consulting the specialist who will prescribe the medications to use and give the indications for the type of currents to use.

The current intensity should be regulated as to be barely perceptible.

DO NOT APPLY THE MEDICATION DIRECTLY TO THE SKIN. Apply the medication to the absorbent surface of the electrode corresponding to the medication's polarity; the absorbent surface of the other electrode should be dampened with slightly salted water, to promote conductivity.

- To run the Ionophoresis programs, use exclusively one special gray cable connected to the outlet of channel 1. Either the light gray or dark gray cable may be used.

THE CHAMPION

- The Ionophoresis programs cannot be run in the "2+2 mode" with multiple treatments.
- The IONOPHORESIS programs are memorized in the "Last 10 Executed" menu but cannot be run in AUTO STIM mode.

Because of the presence of clinical programs, this product is a medical device. Therefore it is certified by the KIWA CERMET ITALIA S.P.A. Body n°. 0476 according to 93/42/CEE directive for medical devices. The certification covers clinical applications.

Action Now Program list

Action Now programs are normal EMS programs, with the only difference that each single action will start only after pressing * button. The Action Now programs are particularly useful to link and synchronize the electric stimulation with a voluntary action. This program is suggested mostly in sport field, for athletic preparation. It enables to activate the muscular contraction through an external control managed by an operator. In this way it is possible to link the stimulation to the voluntary contraction to obtain a greater recruitment of the muscular fibers and an important coordinating effect.

Operating mode: contraction will start after pressing * button. To interrupt contraction before contraction time is over, it is enough to press again * button. In this case the program will cut the rest period and will place itself at the beginning of the ramp of the next stimulation, waiting for the user to press * button in order to start contraction.

The following programs are not medical.

Area	Name	Hz	Ramp-Up time	Contraction time
Upper limbs	Action 0,2 - 1 s	30	0,2	1
	Action 0,5- 1s		0,5	1
Lower limbs	Action 1 - 1 s	50	1	1
	Action 2 - 1 s		2	1
Trunk	Action 3 - 2 s	80	3	2
	Action 4 - 2 s		4	2
	Action 2 - 6 s		2	6
TOTAL	84 programs			

CE0476 does not refer to non-medical treatments.

"3S" Serial Sequential Stimulation Program List

The "3S" programs are characterized by an activation delay of the channels 3 and 4 compared with the channels 1 and 2. The Serial Sequential Stimulation permits to stimulate the musculature in kinetic chain thanks to the differentiated activation times of the muscular groups involved.

In aesthetic field, the 3S programs allow to create a real sequential drainage: the sequential contraction of the different muscular groups produces a deep pressure wave in the musculature involved that causes the interstitial fluid drainage and it favors the return of the venous blood to the heart.

OPERATING MODE:

The operation of these programs is exactly the same as any other EMS programs, with the only difference that a delay in contraction start between the channels will be noticed.

The following programs are not medical.

The 3S program list includes 54 parameter combinations.

Area	Name	Hz	Delay time
Upper limbs	SerSeqStim 0,1 s	30	0,1
	SerSeqStim 0,2 s		0,2
	SerSeqStim 0,3 s		0,3
Lower limbs	SerSeqStim 0,5 s	80	0,5
	SerSeqStim 1 s		1
	SerSeqStim 2 s		2
Trunk	SerSeqStim 3 s		3
	SerSeqStim 4 s		4
	SerSeqStim serial		11
Total	54 Programs		

"Delay time" refers to the delay seconds that the next pulse needs to start.

CE0476 does not refer to non-medical treatments.

GENERAL NOTES ON ELECTRODE POSITIONING

Correct electrode positioning and size choice are fundamental to assure the effectiveness of electrostimulation.

To choose the size of the electrodes and their positioning it is necessary to refer to the images at the end of this manual. Information is also available on our website www.globuscorporation.com.

N.B. For all the programs that cause significant muscle contraction (e.g. strength, hypertrophy, toning and firming programs) it is fundamental to place the electrode on the muscle **motor point**, which is the most sensitive to stimulation.

If the electrode is not positioned exactly on the motor point, the contraction could be small and/or annoying. In this case it is necessary to shift the positive electrode of a few millimeters to feel an effective and comfortable muscle contraction.

Body position during stimulation


Body position during electrostimulation depends on the body part involved and on the type of program that is being carried out.

During high-intensity treatments, we suggest blocking the limbs in order to work isometrically. For instance, if you want to treat quadriceps with a strength program, we suggest to carry out the treatment in a sit position and block the feet, in order to avoid involuntary leg extension during the contraction.


For all the programs that do not imply high intensity (massages, decontracting, drainage...) the body position is not important, as long as it is comfortable.

Electrode positioning for Tens and Microcurrent programs

In the following pages of this manual you can find the images with the correct electrode positioning for tens and microcurrent treatments. If the localization of your pain type is not included among the images, you can place the electrodes by forming a "square" on the aching area. Here you have an example.

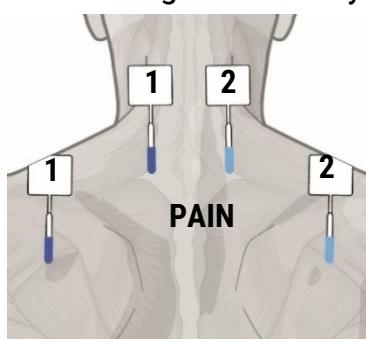

TENS (use
colored cables)

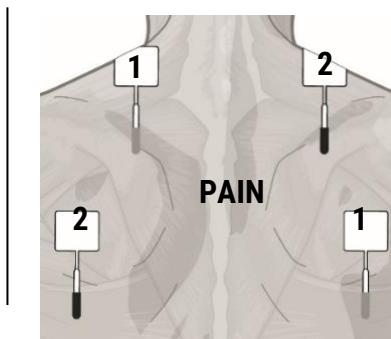

**MICRO -
CURRENTS**
(use gray cables)

Indications for the use of ionophoresis

This program uses a low-intensity and continuous current (between 5 and 10 mA) that helps the absorption of the active ingredients of a drug in a specific area of the body. It is often required that a drug is administered directly on the area that needs to be healed, avoiding an oral or intravenous administration. With ionophoresis it is possible to administrate a drug through transcutaneous penetration directly on the body area that needs to be treated.

The drug must be prepared in ionic form and must have an electric charge. The principle on which ionophoresis is that the continuous current flows through skin from one electrode to the other (from anode to cathode) consequentially transporting the electrically charged iones that are inside the treated body area.

In practice, sponges soaked in a solution containing the active ingredient are used, bearing in mind that if it has a negative charge, it must be applied to the negative electrode and vice versa. The current will carry the active principle inside the tissues, because the ions of the active principle itself will migrate towards the opposite pole until the product is completely absorbed. The kit with sponges and electrodes for ionophoresis is an extra accessory that can be purchased separately.

The intensity value is adjustable from a minimum of 0 mA to a maximum of 10 mA.

To ensure safety, the maximum intensity, calculated with the smallest ionophoresis electrodes (50 x 50 mm), is 0.40 mA per cm^2 of electrode.

DENSITY = Current displayed in mA / Electrode area in cm^2


Indications for the application:

- The manufacturer declines the responsibility of the prescribing physician for the choice of the drug to be used with ionophoresis. For this purpose, in this user manual the manufacturer provides the data for a correct definition of the protocol and the drug that has to be used.
- Before using ionophoresis, therefore, it is mandatory to contact the prescribing doctor.
- Both sponges in the ionophoresis kit must be wetted with distilled water or physiological solution, then insert the silicone electrodes inside the sponges and connect the cables.
- The drug used for the therapy should never be applied directly on the skin but to the absorbent surface of the electrode corresponding to the polarity of the drug itself. In fact, it is very important to consider the positive or negative charge sign of the active ingredient of the drug, which must be applied correctly: the drug must be placed on the electrode with the same charge sign as the active ingredient.


THE CHAMPION

- Place the two electrodes on the area that must be treated, at a distance of about 10-20 cm and fix them with the elastic band.
- Gradually increase the intensity until the patient feels a slight tingling.
- Once the program is finished, turn the device off, and disconnect the electrodes. Clean the sponges and bands following the instructions on the drug leaflet. If not indicated, it is however recommended to wash the sponges and elastic bands very well, with plenty of hot water and soap, so that the next time there are no traces of the drug.


ELECTRODE POSITION

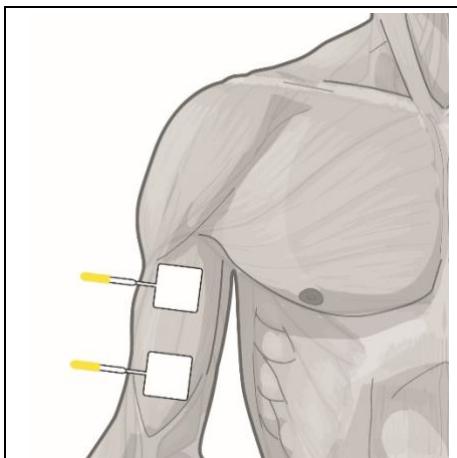


Biceps brachii

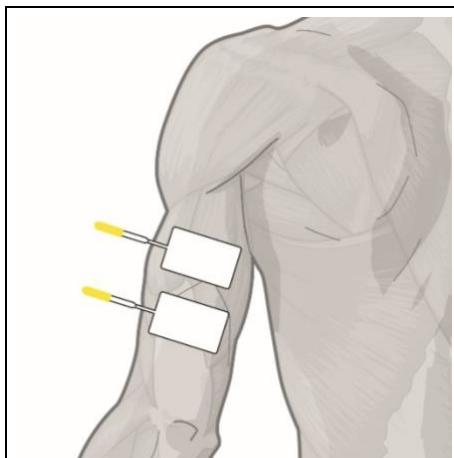


Triceps brachii

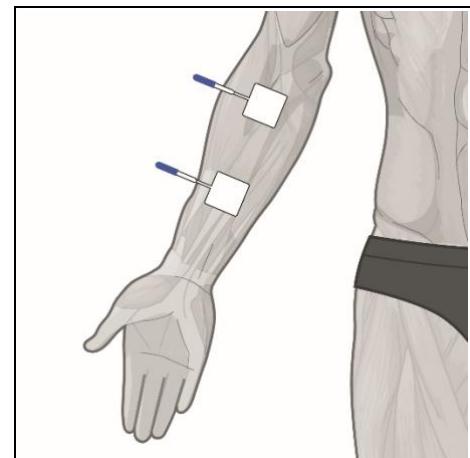


Flexor carpi

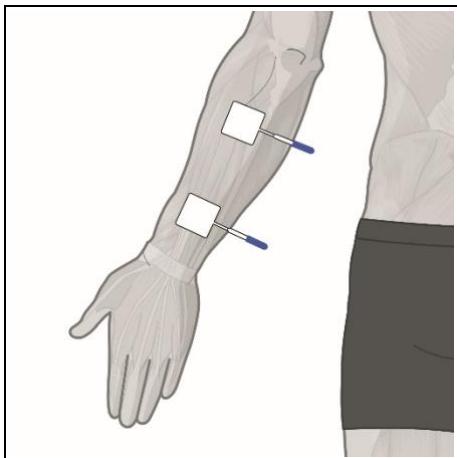


Extensor carpi

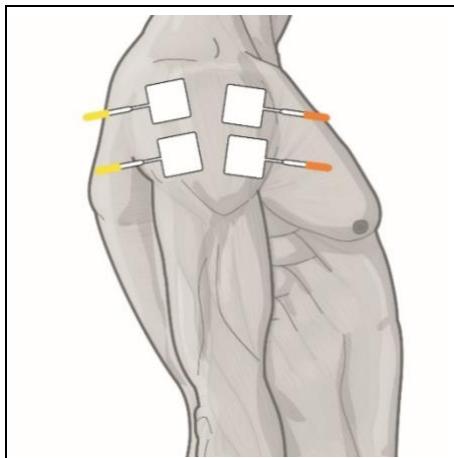


Deltoid

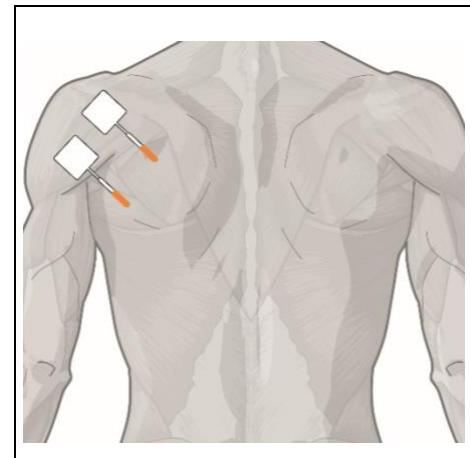


Posterior deltoid

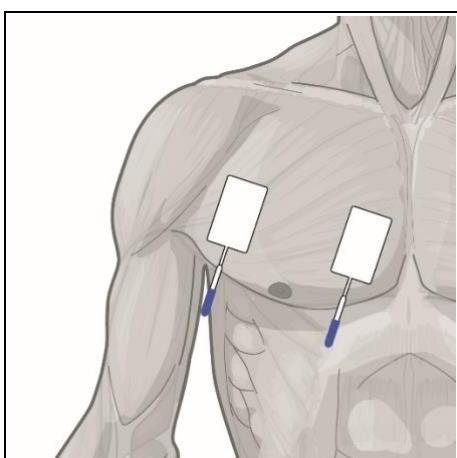

Pectoral

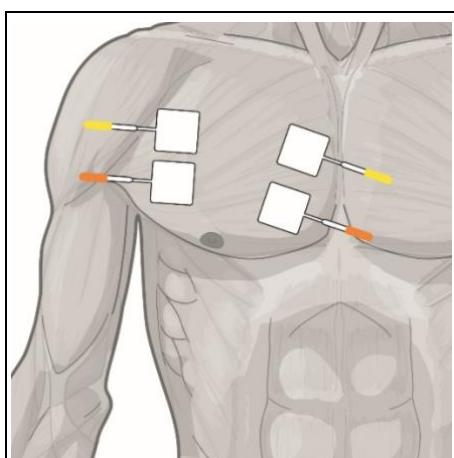


Pectoral

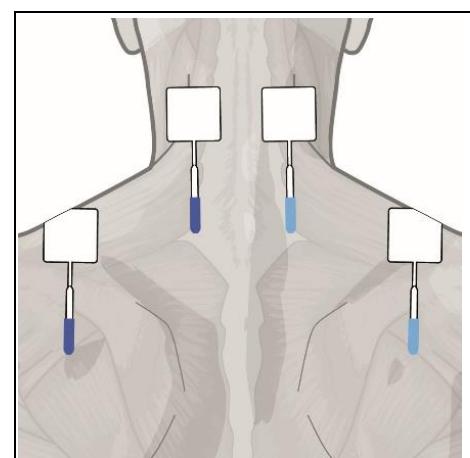


Trapezius


ELECTRODE POSITION

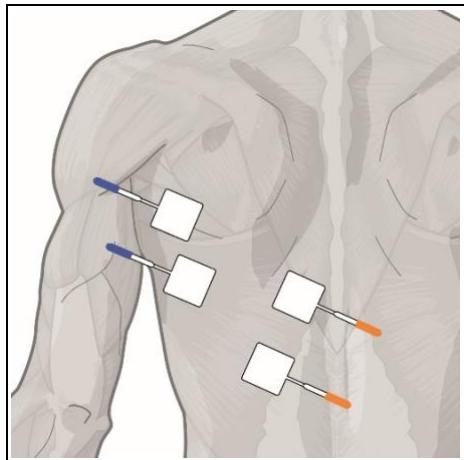


Latissimus dorsi

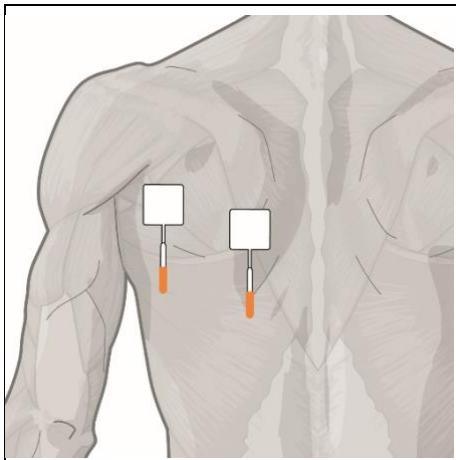


Infraspinatus

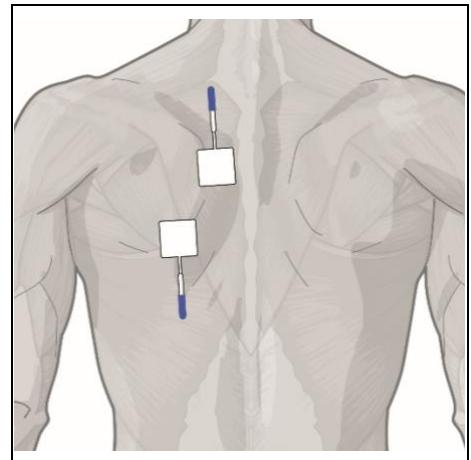


Rhomboid

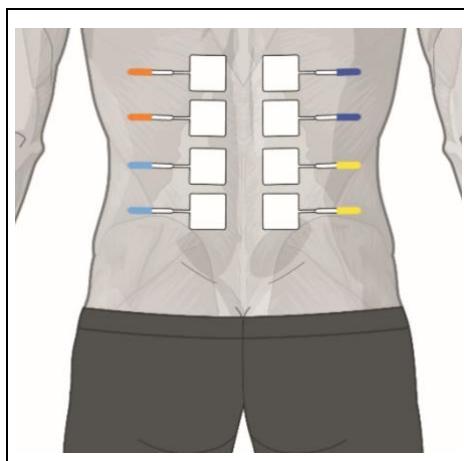


Lumbar/Dorsal muscles

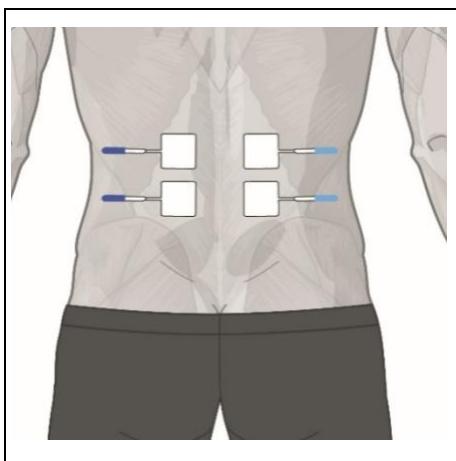


Lumbar muscles

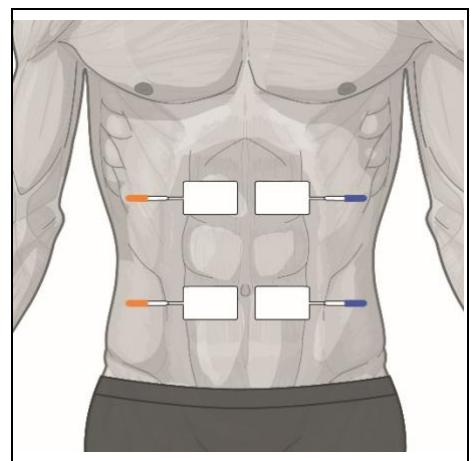


Abdominals

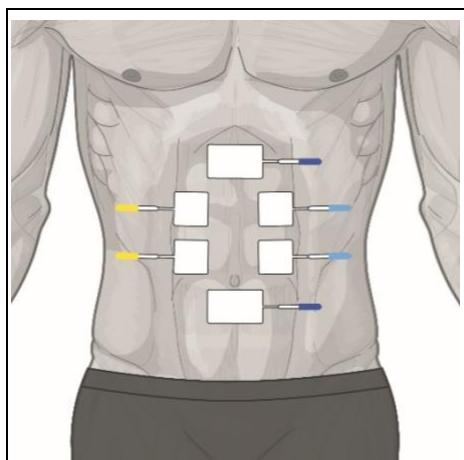

Rectus abdominis

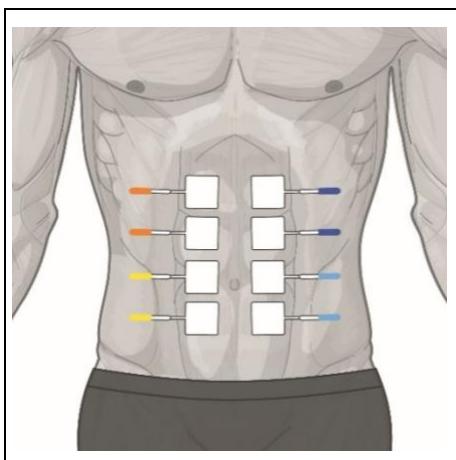


Rectus abdominis

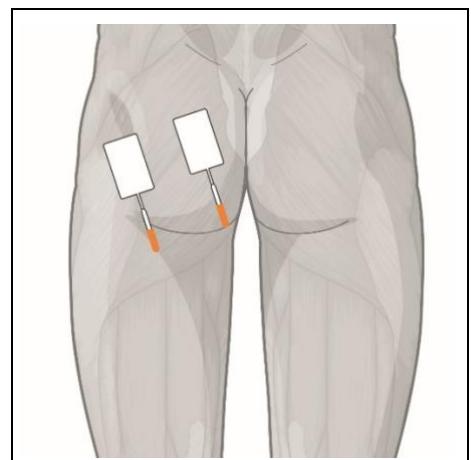


Gluteus


ELECTRODE POSITION

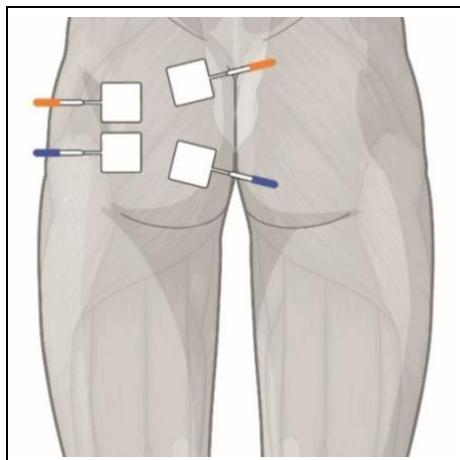


Gluteus

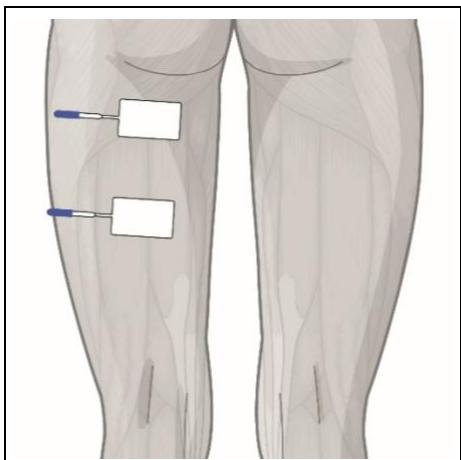


Hamstrings

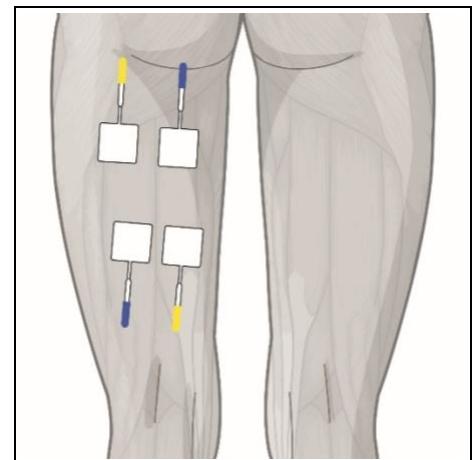


Hamstrings

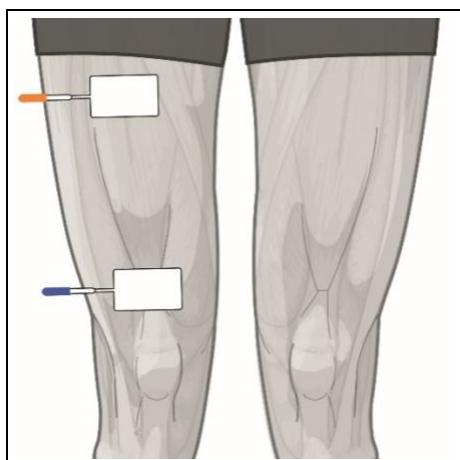


Quadriceps

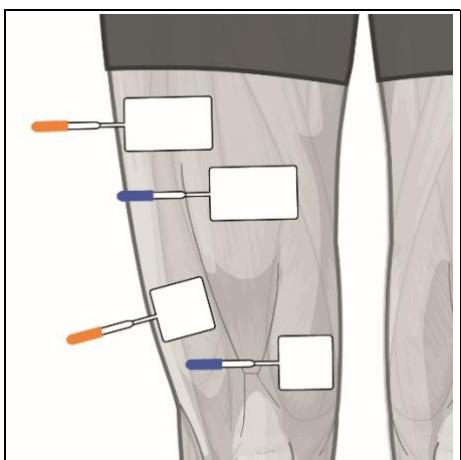


Quadriceps

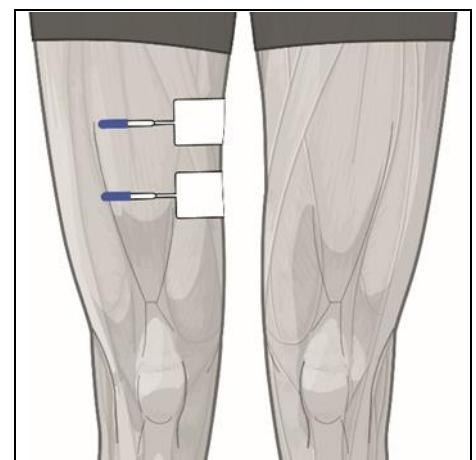


Adductors

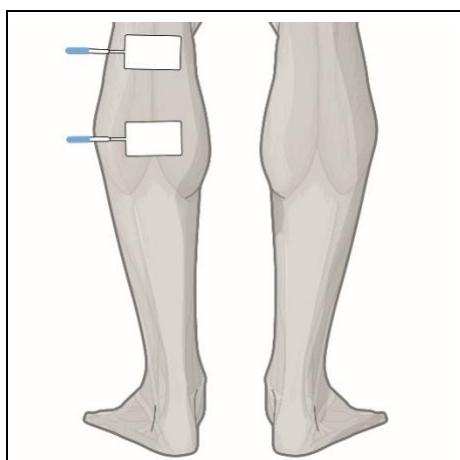

Calf

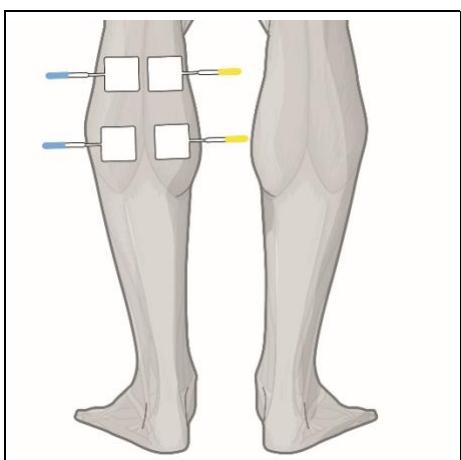


Calf

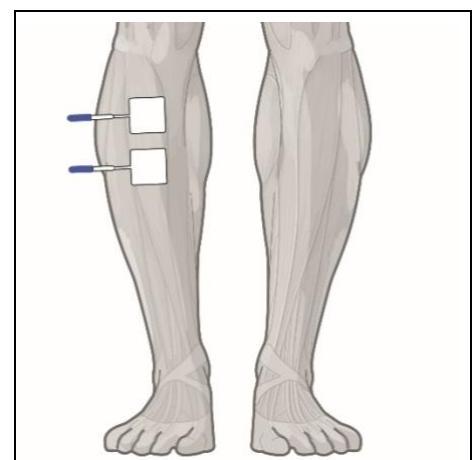


Tibialis anterior


ELECTRODE POSITION (TENS)

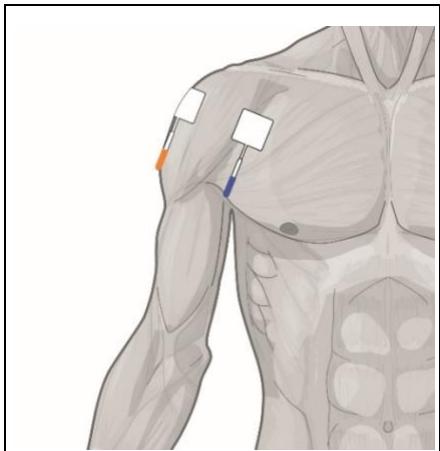


Anterior shoulder pain

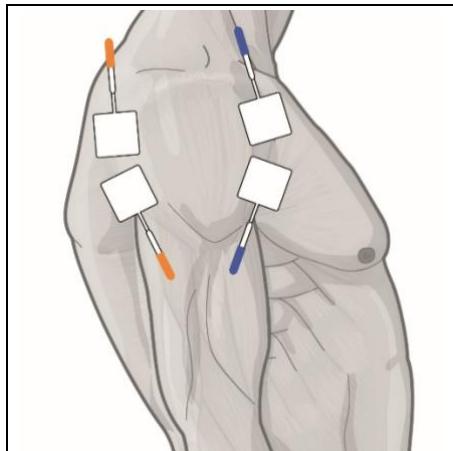


Shoulder pain

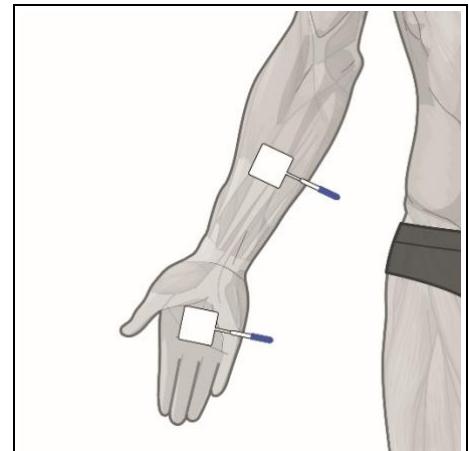


Carpal tunnel

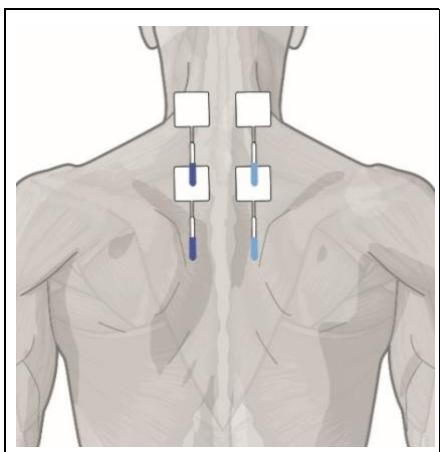


Neck pain/Whiplash

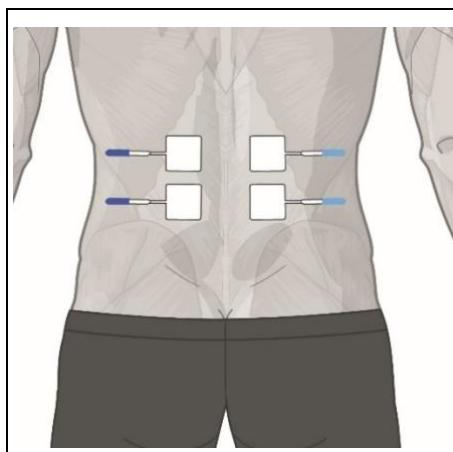


Chronic low back pain

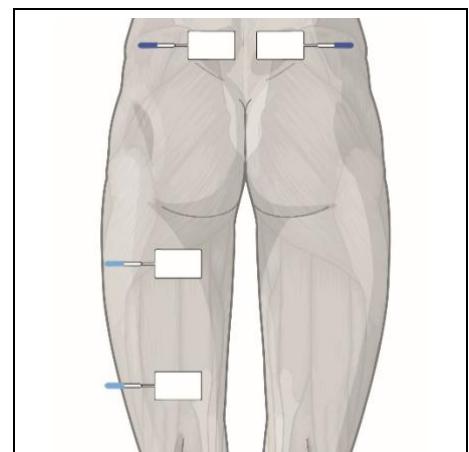

Sciatica

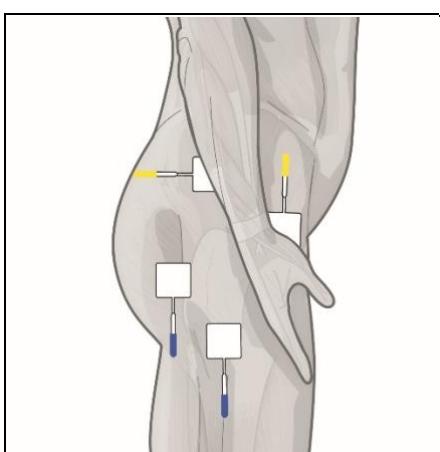

Coxarthrosis

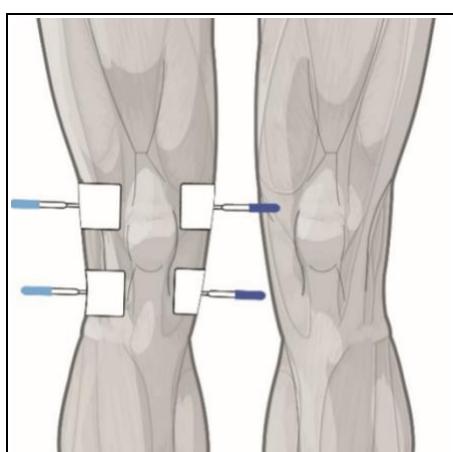


Gonarthrosis/Knee pain




Ankle joint arthrosis


MICROCURRENT ELECTRODE POSITIONING

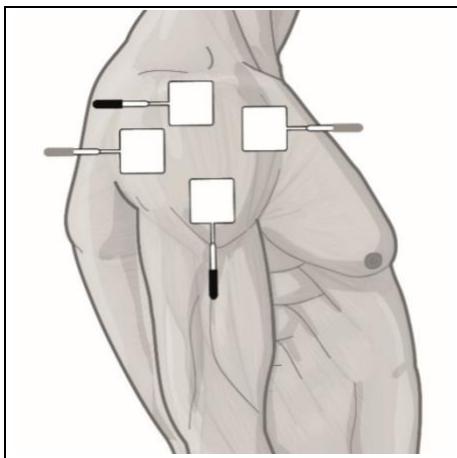


Shoulder dislocation

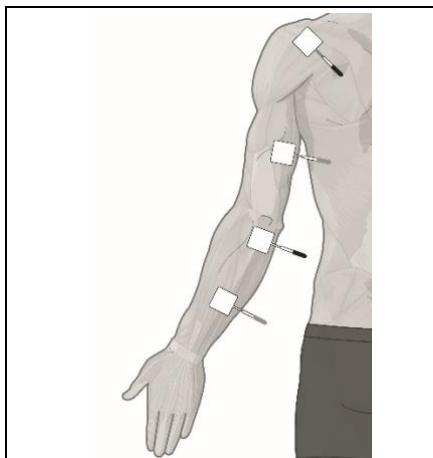


Brachialgia

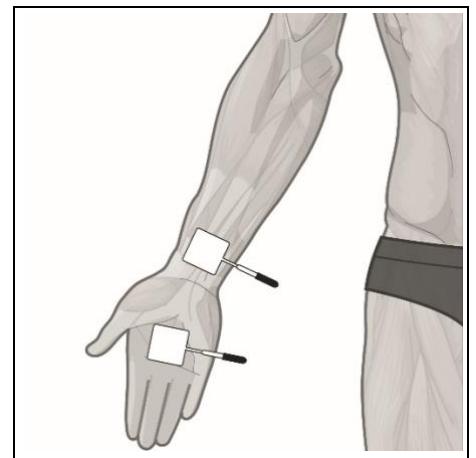


Carpal Tunnel

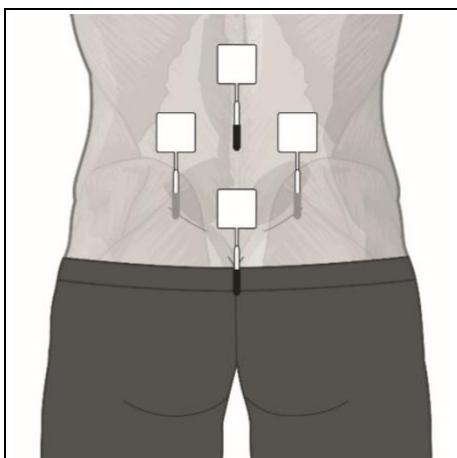


Low Back Pain

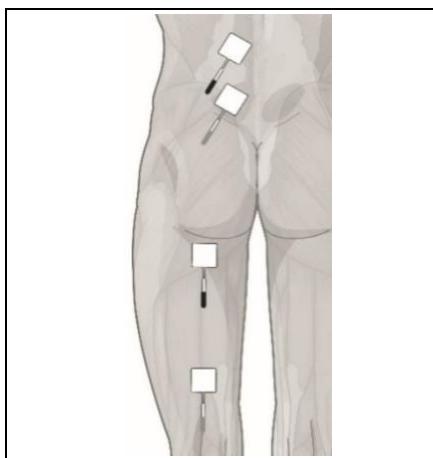

Sciatica

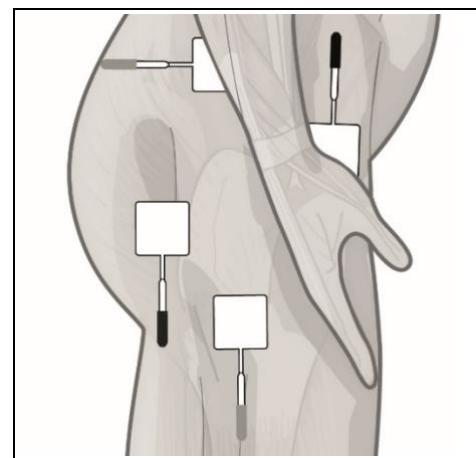

Hip pain

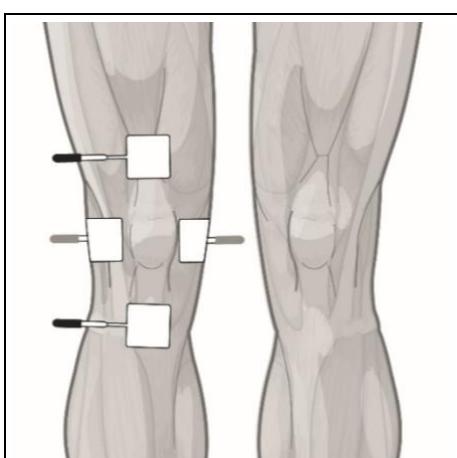

Knee Osteoarthritis



Achilles Tendinopathy



Sprained ankle

ACTION PRINCIPLES

Muscular electrostimulation

Electrostimulation is a technique that, by means of electric pulses that act on the muscle motor points (motoneurons), causes a muscular contraction similar to voluntary contraction.

The majority of human muscles are striated or voluntary, with approximately 200 muscles on each side of the body. (about 400 on the whole)

The physiology of muscular contraction

The skeletal muscle performs its functions through contraction. When a movement is made, the motor center of the brain sends an electric signal to the muscle to be contracted.

When the electric signal reaches the muscle, the motor plaque of the muscle surface produces the depolarization of the muscle membrane and the release of Ca^{++} ions inside it. The Ca^{++} ions, interacting with the actin and myosin molecules, activate the contraction mechanism which leads to the shortening of the muscle.

The energy required to contract the muscle is provided by adenosine triphosphate (ATP) and supported by a recharging system based on aerobic and anaerobic mechanisms using carbohydrates and fats. In other words, electrostimulation is not a direct source of energy, but it acts as a tool triggering muscle contraction.

The same principle is activated when muscle contraction is generated by EMS, which act as a natural impulse transmitted by the motor nervous system. At the end of the contraction, the muscle relaxes and returns to its original state.

Isotonic and isometric contraction

An isotonic contraction occurs when, during a movement, the muscles overcome external resistance, thus shortening and leading to a constant state of tension in the tendon heads. When external resistance impedes the movement, instead, muscle contraction does not cause muscle shortening, but increases the intensity at muscle heads: this condition is called isometric contraction. Isometric stimulation is normally used in electrostimulation because it generates a more powerful and effective contraction.

The distribution of the different fiber types in the muscle

The relationship between the two main categories (type I and type II) can vary in a considerable way.

There are muscular groups that are typically made up of type I fibers, like the soleus,

THE CHAMPION

and muscles which only have type II fibers, like the orbicular muscle; however, the majority of human body muscles is composed of a combination of the two types. Studies on the distribution of fibers in the muscle have highlighted the close relationship between the (tonic or phasic) motoneuron and the functional features of the fibers it innervates; moreover, they have proved that a specific motor action (particularly in sports) can lead to a functional adaptation of fibers and change their metabolic features.

Motor unit type	Contraction type	Contraction frequency
Tonic ST	slow contraction I	0 - 50 Hz
Phasic FT	fast contraction II	50 - 70 Hz
Phasic FTb	fast contraction II b	80 - 120 Hz

Stimulation intensity

The intensity value required to trigger contraction depends on patients, electrode placement, adipose tissue, perspiration, possible hairs on the treatment surface etc. Therefore, the same current intensity may give different sensations to different people, in different days or body sides. It is advisable to regulate the intensity during the same session to contrast accommodation, in order to obtain the same contraction.

The current intensity for the different phases is suggested with an approximate value and can be modified on the basis of individual sensations.

- Moderate: the muscle does not tire, even during long treatment. The contraction is agreeable and tolerable. First level of the intensity graph.
- Intermediate: the muscle is visibly contracted but the stimulation does not trigger the joint movement. Second level of the intensity graph.
- High: the muscle is contracted noticeably. The muscle contraction would extend or bend the limb if not blocked. Third level in the intensity graph.
- Maximal: the muscle is contracted maximally. This is an intense treatment that should be performed only after many applications.

Moderate	From 10 mA to 20 mA
Intermediate	From 20 mA to 30 mA
High	Above 30 mA
Maximal	<i>On the verge of the tolerance limit, always under the threshold of pain.</i>

In treatment description, recommended intensity levels are indicated.
N.B. Recommended current levels are just an indication.

NOTE: It is not necessary to set the intensity value (in mA) in Microcurrent programs, since it has already been set for all the phases.

Open circuit

This device includes a controlling device of power emissions. If the operator increases the intensity level above 10 mA and the circuit is open (cables are not connected to the device and electrodes are not applied to the skin), the electrostimulator immediately resets the intensity to 0 mA.

Therefore, before starting a program, make sure that the cables are connected to the device and that the electrodes are placed on the area to be treated and that they are not worn, as this could decrease their conduction capacity. NOTE: Use the Microcurrents programs only on channels 1 and 3 with the gray cables. If the cables are not connected or they are of the wrong type, the program will not start. Check the cables and the connections.

Tens

Transcutaneous Electrical Nerve Stimulation (TENS) is a selective stimulation of the large fibers of the peripheral nerves favoring the closing of the gate entrance for the pain pulses and increasing the release of endorphin substances, reducing in this way the pain intensity. Therefore TENS is particularly indicated to treat the severe and chronic pain caused by the main musculoskeletal disorders.

TENS currents reduce pain thanks to the following factors:

- a. Gate control theory
- b. Endorphin secretion
- c. Different sedative effects related to frequency

Gate theory

If the electrical signals that lead to the brain information about pain are stopped, also the perception of pain is eliminated. For instance, if we hit our head against an object, the first thing we do is massaging the traumatized area. In this way we stimulate the receptors of touch and pressure. TENS in continuous mode and frequency modulation can be used to generate signals similar to those of touch and pressure. If their intensity is sufficient, their priority is so high that it prevails on the pain signals. When the priority is obtained, the gate of sensory signals is opened and the pain gate is closed, impeding the passage of these signals to the brain.

Endorphin secretion

When a nervous signal proceeds from the pain area to the brain, it spreads through a chain of connections joined together called synapses. The synapse can be seen as the space between the end of a nerve and the start of another. When an electric signal reaches the end of a nerve, it produces substances called neurotransmitters that pass through the synapse and activate the start of the next nerve. The process is repeated until the signal reaches the brain. The opioids involved in pain reduction have the task of sliding in the synapse space and impeding the neurotransmitter propagation. In this way a chemical block of pain signals is obtained. The endorphins are opioids naturally produced by the body to tackle pain and they can act both on the marrow and on the brain, proving to be effective analgesics. Tens can increase the natural production of endorphins; therefore they decrease the perception of pain.

Different effects related to frequency

Higher frequencies determine immediate, short-lasting antalgic effects, whereas lower frequencies determine gradual, long-lasting effects.

Microcurrents

Unlike conventional electrostimulation, which uses electrical current in the milliampere (mA) range, microcurrent electrostimulation uses currents with an intensity included between 10 and 500 μ A (microamperes, that is a millionth of an ampere). Several studies have proved that microampere currents actually increase ATP synthesis.

MENS therapy usually has two different phases: the first aims at reducing the pain sensation perceived by the patient, while the second promotes protein and ATP synthesis, accelerating tissue repairing processes. Usually the treatment duration is included between 15 to 30 minutes as for the first phase and between 5 and 10 minutes as for the second phase. MENS are an interesting instrumental therapy that can be used in a lot of pathologies; moreover, the use of MENS combined with other instrumental therapies such as laser and TENS can lead to excellent clinic results, which are otherwise unlikely to be reached.

Ionophoresis

Ionophoresis is a form of electrotherapy through which pharmacological substances are transmitted inside the tissues thanks to a unidirectional continuous electric current. Ionophoresis is based on the ionic dissociation capacity of some medicinal substances, which have very low molecular weight, after they are dissolved in water.

It is crucial to know if the active part of the medicine, after being dissociated in a ionic form, has positive or negative charge, with the aim of placing it correctly according to the direction of the electric flow.

The ions of the medicinal substance are transmitted inside the organism through cutaneous areas that oppose a low resistance to the current, reaching the cellular membranes that are thereby electrically modified.

MAINTENANCE AND CLEANING

Device

- In case of actual or alleged malfunctioning, do not tamper with the device and do not try to repair it by yourself.
- Do neither intervene on the device nor open it. Only specialized and authorized centers can repair it.
- Avoid violent impacts that may damage the device and cause malfunctioning, also not immediately detectable.
- Use this device in a dry and open environment. Do not wrap the device.
- Clean the device only by using disinfectant with sodium hypochlorite or quaternary ammonium salt (percentage: 0.2-0.3%) diluted with distilled water. After cleaning/disinfecting the device, dry it perfectly with a clean cloth.
- It is recommended to clean/disinfect the parts after every use, unless otherwise indicated.
- Always use the device with clean hands.
- It is recommended to use the device in a clean environment to avoid contamination with dust and dirt.
- It is recommended to use the device in a ventilated, well-aired space.

Battery

Battery management

The device has a menu that allows to see the status of the battery charge, if the device has one. The values displayed in this menu enable the manufacturer and/or the authorized help center to check the status of the battery charge.

Accessories

Use and storage of the electrodes and the cables

In case of damaged cables or electrodes, these should be replaced and not used anymore.

THE CHAMPION

Before placing the electrodes on the skin, we suggest to clean it accurately. After using the multi-purpose single patient and/or single-use electrodes, they must be stored using their plastic film and placed in a clean closed plastic bag.

Electrodes should not touch each other nor overlie one over the other.

Once the package has been opened, the electrodes can be used for 25-30 applications. The electrodes must always be replaced if they do not stay perfectly in contact with the skin.

If using non self-adhesive electrodes it is suggested to clean their surface with proper cleansers that respect the requirements described in the manual.

Use the electrodes with clean hands.

The electrodes in their bag should be stored in an environment that respects the requirements described in the manual.

At the end of the treatment, unplug the cables from the connectors and clean them carefully with proper cleansers that respect the requirements described in the manual.

After cleaning and drying them, fold them up and place them in the plastic bags supplied along with the cables.

WARRANTY

The device is guaranteed to the first user for twenty four (24) months from the purchase date against material or manufacturing faults, twelve (12) months if the device is used for professional purposes, provided that it is used properly and maintained under normal operating conditions.

Warranty coverage is limited in the following cases:

- six (6) months for supplied accessories subject to wear, such as batteries, battery chargers, power supply units, cables, G-Trode handpiece.
- ninety (90) days for the media containing software such as, for example, CD-ROMs, memory cards, etc.
- The warranty does not cover "consumer" accessories and materials such as the electrodes, etc.

The warranty is valid and enforceable in the country where the product was purchased. In the event that the product is purchased in an EU country, the warranty is valid in all the member states.

In order to take advantage of the warranty service, the user must comply with the following warranty clauses:

1. Products have to be sent for repairs by and at the expenses of the Customer in their original packages and with full original equipment.
2. The warranty of the product is subject to the exhibition of a fiscal document (sales

receipt or invoice) attesting the purchase date of the product.

3. The repair work shall have no effect on the original expiry date of the warranty and shall neither renew nor extend it.

4. If no defect is found, when it comes to carrying out the repair work, the costs of check time will be charged in any case.

5. The warranty becomes void if the flaw has been caused by: impacts, falls, misuse of the product, use of non-original power supply units or external chargers, accidental events, alteration, replacement/detachment of the warranty seals and/or tampering. Moreover, the warranty does not cover damages caused during transportation when unsuitable packages are used (see point 1).

6. The warranty does not cover the inability to use the product, other incidental or consequential costs or other expenses incurred by the purchaser.

N.B. Before returning the device for repairs, we recommend reading carefully the user instructions in the manual and visiting the Globus website. If you have to return the product for repair, please contact your dealer or the Globus customer service.

FAQ

What kind of electrodes should be used for electrostimulation?

The use of adhesive electrodes is recommended, because they are more practical and improve stimulation quality. If used with care, i.e. on clean skin, they can be used for up to 25-30 applications. The electrodes must always be replaced if they do not stay perfectly in contact with the skin.

Where should the electrodes be placed?

This manual reports the images of electrode positioning for all body parts. (respecting the indicated polarity is not necessary) It is sufficient to follow these instructions.

To verify the correct placement of the electrodes, use the special Motor Point Pen or follow this empirical method: place the electrodes as indicated in the pictures; start the stimulation; with your hand, slide the electrode in different directions on the muscle area. You will notice an increase or a decrease of the stimulation depending on the electrode position. Once you locate the point of highest stimulation, decrease channel intensity to zero (0.0 mA), place the electrode again and increase intensity gradually.

Do Y cables permit to use more electrodes on the same channel?

This allows you to work, for example, on quadriceps vastus medialis and vastus lateralis with the same channel; you can use both split cables to treat two limbs simultaneously, involving 4 muscles. Do not use them for medical applications.

Does power decrease using splitted "Y" cables?

THE CHAMPION

The power intensity of each channel does not vary. However, when Y cables are used to split one channel, the current is distributed on a wider muscle area, therefore the contraction will be weaker. Increase the intensity to obtain the same contraction.

Can electrostimulation hurt?

Muscle damage is very unlikely. An important principle that should be followed is to increase intensity gradually, observing muscle behavior and avoiding to keep the limb completely outstretched. In case of doubt, please contact a specialist.

Is it possible to use the electrostimulator during menstrual cycle?

Possible interferences, such as anticipation, delay, accentuation or reduction of the cycle are extremely subjective and variable. In any case, it is recommended to avoid treatments in the abdominal area during menstrual cycle and immediately before or after it.

Is it possible to use the electrostimulator during lactation?

Until now, no collateral effects regarding lactation have been observed. Nonetheless, during lactation, it is recommended not to stimulate the thoracic region.

Are dermatological diseases (e.g. psoriasis, urticaria) contraindications for electrostimulation?

Yes, do not treat skin areas affected by serious dermatological diseases.

When are the first results visible?

The aesthetic results of electrostimulation are always subjective.

However, it is possible to say that, in the case of tonification, 3-4 regular and constant weekly sessions can already bring good results after 15 days, while electrolipolysis and electrodrainage require 40 days. It is possible to obtain better and quicker results if treatments are combined with good physical activity and a correct life style.

How many sessions can be performed on a weekly basis?

As regards physical training sessions, we recommend to follow the technical guide available on Globus website. As regards fitness and beauty, the number of sessions depends on the type of treatment. 3-4 sessions per week on alternate days are suggested for toning. Daily treatments are permitted for lipolysis and drainage programs.

EMC accompanying documents

Essential performance

PERFORMANCE	CONDITION	RISK	ACCEPTED EVENT
Electrostimulation.	External disturbance (Burst).	Display information no longer readable.	The device must stop the stimulation.
			The device must maintain the stimulation and accept the commands.
	Lack of internal power supply.	Interruption of the treatment.	The machine must signal the battery exhaustion and the interruption of the treatment.
	Lack of external power supply.	Interruption of the treatment.	The device, if equipped with a battery, must continue the treatment signaling that operation is carry out in battery mode.
	Detachment of an electrode.	Unpleasant stimulation or painful electric shock in case of reconnection of the electrode.	The device must constantly monitor the current on each active channel set over 9 mA. In case the detected current is below a certain threshold, the machine must rest the current of the channel.
	The cable for microcurrents is not detected.	Dangerous stimulation.	The device must report an error relating to the electrodes and prevent the program from starting.
	Setting of a current that is too high in case of microcurrents.	Dangerous stimulation.	The device must derate the voltage boost stage to prevent emitting a current beyond the maximum value.

THE CHAMPION

			The device must not start the microcurrent treatment if it does not detect the hardware derating of the voltage booster stage.
Loading of the programs from the memory.	Error in the data from the memory.	Execution of an incorrect program.	The machine must check the correctness of the data of the programs. In case an error is detected, the device must restart.
Change of settings.	Setting data memory error.	Operation error.	The device must check the correctness of the settings data and in case of errors it must load the default settings present in copy in the memory and must indicate on the display that the reset has been carried out.
		Display information no longer readable.	The device must check the contrast value. If it is out of range, the device must reset the value to the default one.
Battery charge.	Battery overheating.	Damaging of the device, display information no longer readable, explosion, fire.	The device must monitor the temperature of the battery, if a certain threshold is exceeded, the battery charging must be interrupted.

In compliance with:

EN 60601-1: 2006 + A1: 2013

EN 60601-1-2: 2015

EN 60601-2-10: 2015

EN 60601-1-11: 2015

Warning: radiofrequency communication devices (including accessories like antennas or antenna cables) must be used at least 3 meters away from every part (including cables and accessories) of the device. Otherwise performance can be affected.

THE CHAMPION

THE CHAMPION